

Fig. 1

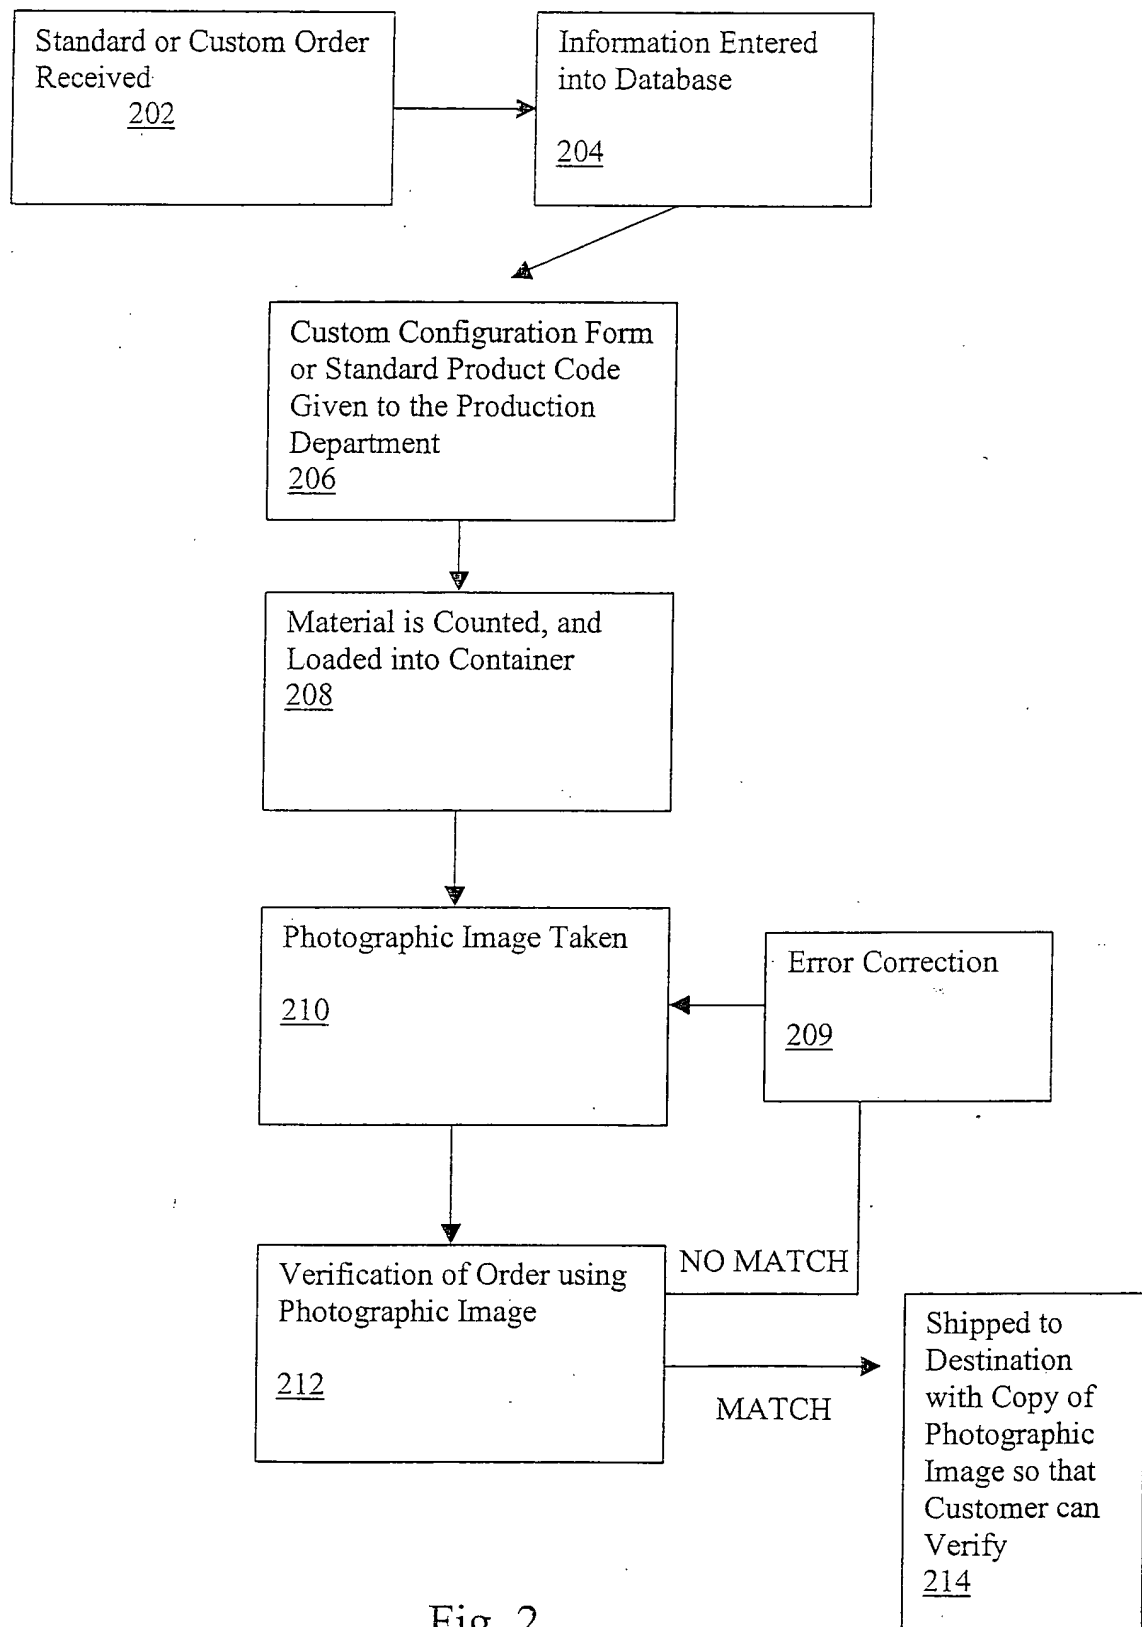


Fig. 2

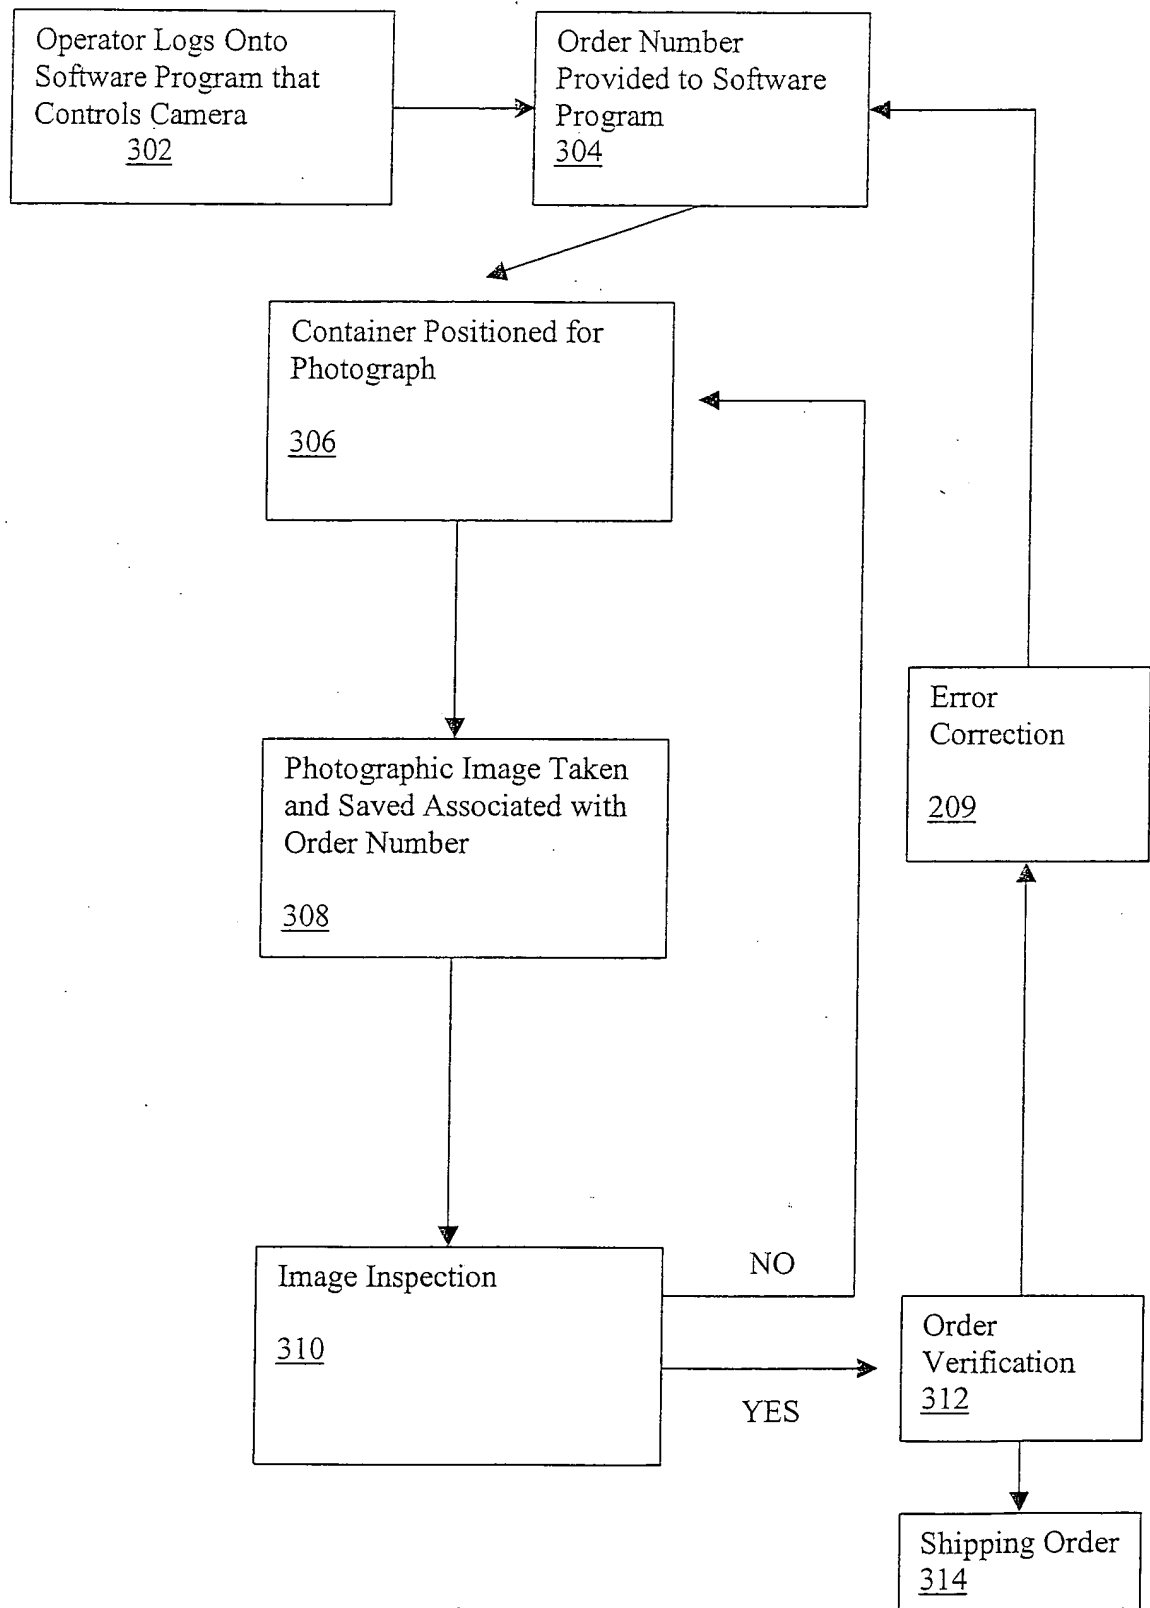
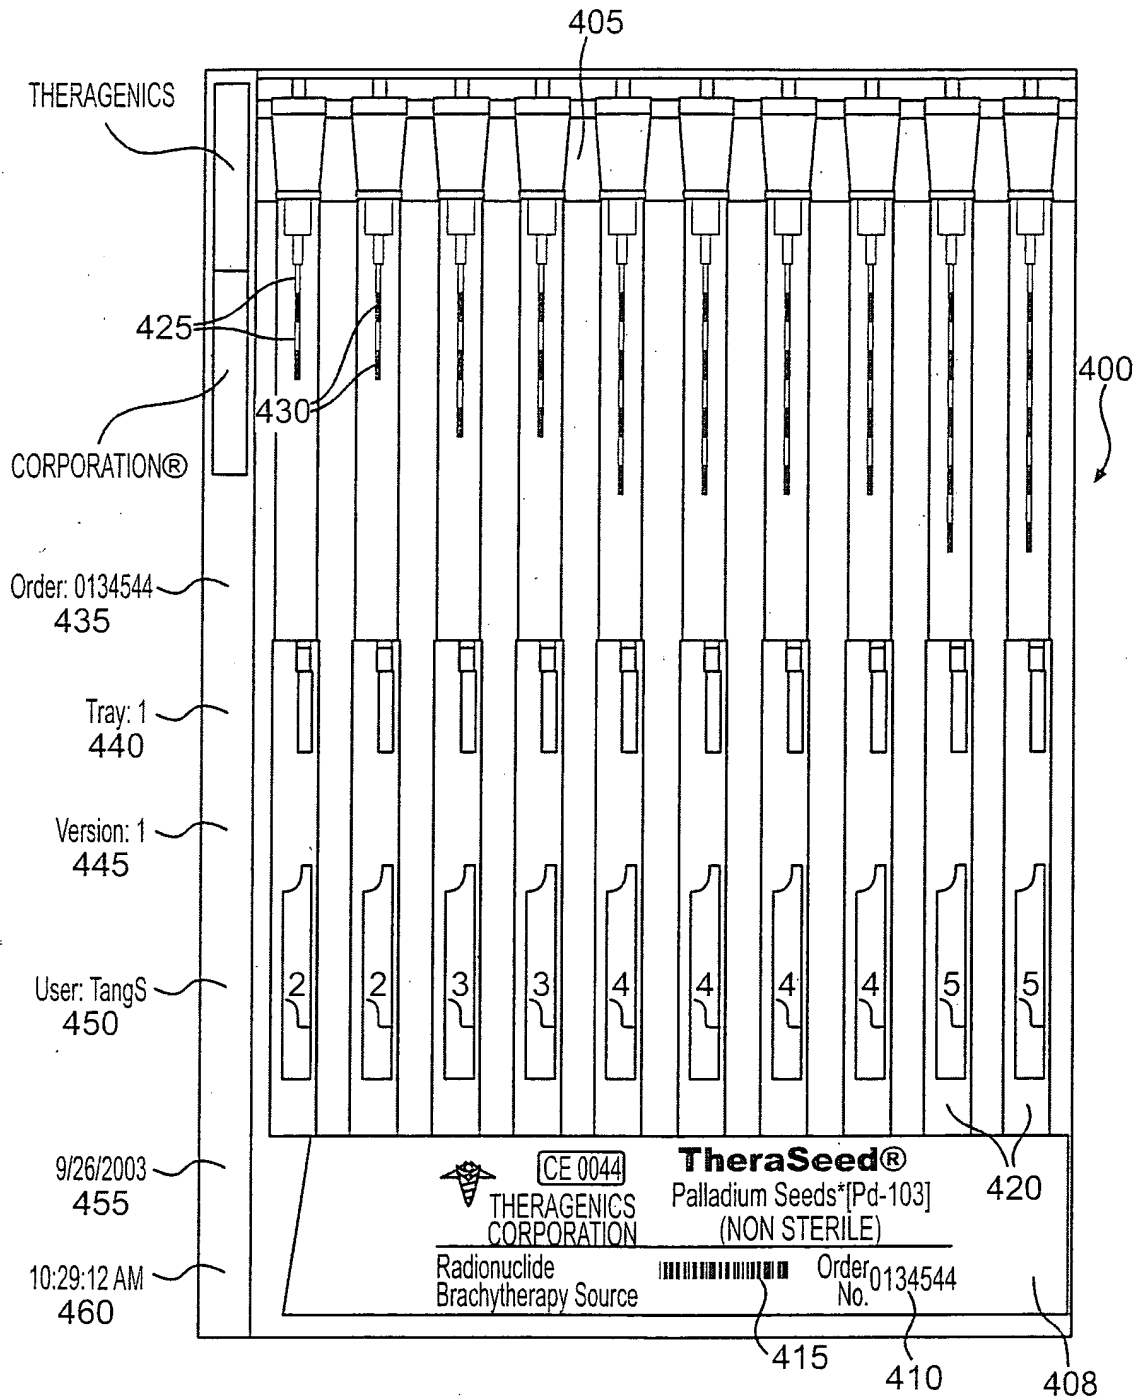


Fig. 3

# Replacement Sheet





**FIG. 4**

## Needle Configuration Form

Ship Date:

Needle Number	Product Code	Number of Spacers	Number of Seeds
Tray 1			
1	TS222	2	2
2	TS224S	2	4
3	TS222	2	2
4	TS222	2	2
5	TS224	4	4
6	TS223S	6	3
7	TS222	2	2
8	TS224	4	4
9	TS222	2	2
10	TS222	2	2
Tray 2			
11	TS222S	8	2
12	TS223S	5	3
13	TS223	3	3
14	TS224	4	4
15	TS223S	7	3
16	TS223S	7	3
17	TS224	4	4
18	TS222	2	2
19	TS222	2	2
20	TS222	2	2
Tray 3			
21	TS223	3	3
22	TS222	2	2
23	TS222	2	2
24	TS222	2	2
25	TS222	2	2
Totals		83	66

Product Code	Number of Seeds
TS200	
TS202	
Totals	0
Grand Totals	83

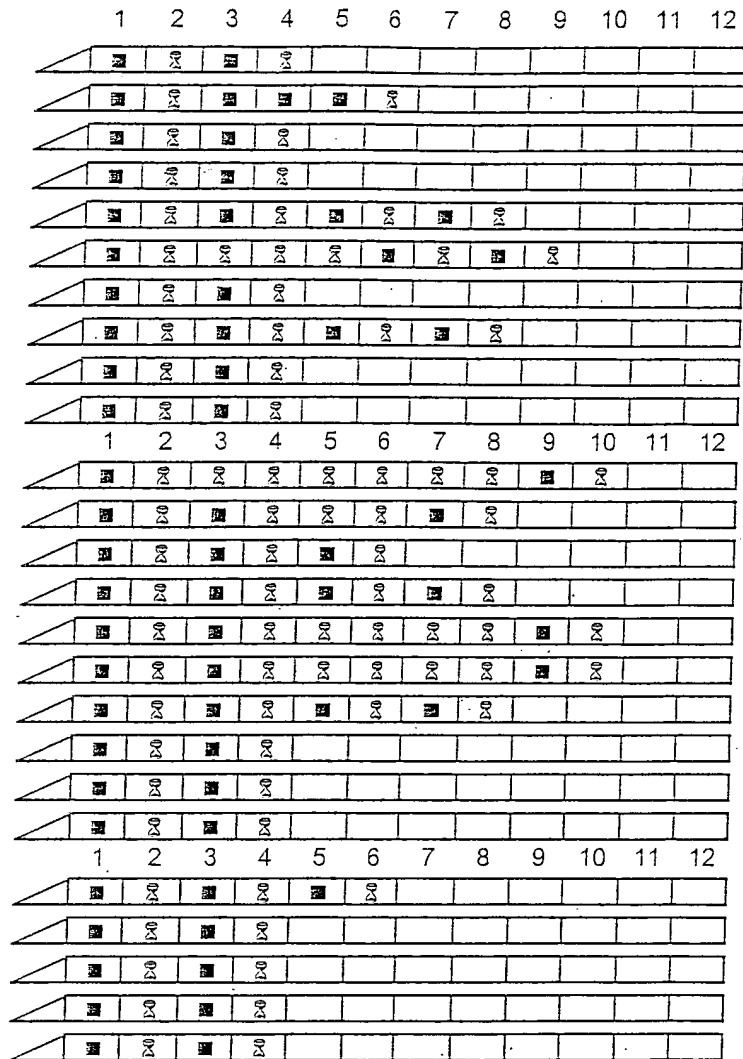

Facility:

Radiation Oncologist:

Implant Date:

Patient Name:

Translator:

Verifier:

Scheduling:

TGX Order #:

This package insert is designed to provide a description of the seed and spacer configuration as ordered by the customer. The health care professional must verify seed/spacer configuration prior to the procedure.

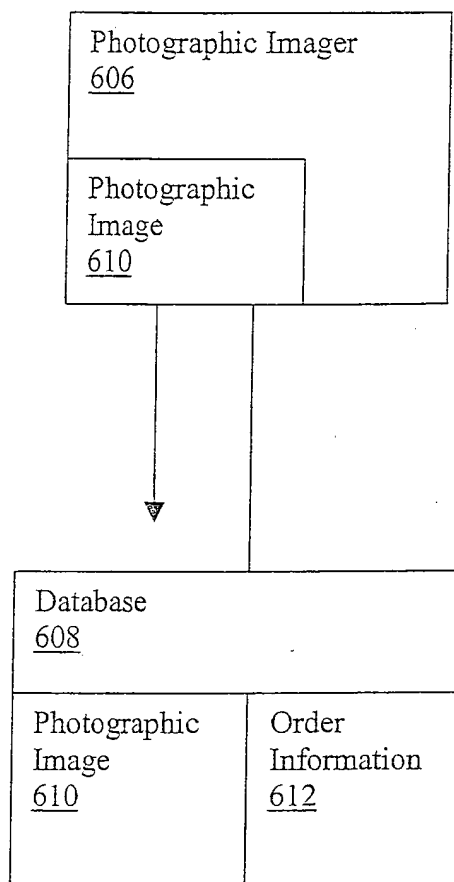
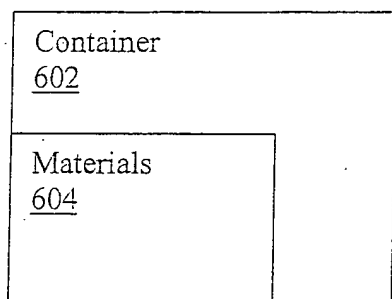


Fig. 6